

# Do international standards for hygienic hand rubs reflect realistic usage?

## INTRODUCTION

Hygienic handrubs are widely used in healthcare to reduce the likelihood of pathogens being disseminated via the hands. International standards such as EN1500<sup>1</sup> have been developed to assess the efficacy of handrubs claiming antimicrobial action. This standard compares a reference product (2x3ml applications of 60% v/v isopropanol (IPA) over 60 seconds) with a test product(s). However, as WHO guidelines<sup>2</sup> recommend that drying times of alcohol-based handrubs (ABHRs) be limited to 30 seconds, one has to ask whether the standard represents realistic usage?

## OBJECTIVE

This study compared the volumes of ABHR applied, drying time, antimicrobial efficacy and user acceptability. The ABHR's studied were 60% v/v IPA and the two WHO-recommended ABHR formulations i.e. WHO1 - 80%v/v ethanol and WHO2 - 75% v/v IPA, both of which contain 1.45% v/v glycerol.

## METHODS

**Drying time and acceptability as a function of volume:** Fifteen volunteers were recruited to test six volumes of the three ABHR's, ranging from 0.5ml to 3ml. The alcohol was applied to volunteers' hands with a calibrated pipette, and rubbed in using the standard hand rub procedure as described in EN1500 (the Ayliffe technique). Volunteers self-reported when their hands were dry; the time from application was recorded. At the end of the test, the volunteers were asked to rate the time taken to dry on a three point scale: too short, OK, too long.

**Antimicrobial efficacy:** Five of the volunteers subsequently applied the same six volumes of the three ABHR's in the manner of an EN1500 test. This involved washing the hands in a non-microbicidal standard soft soap, followed by immersion to the mid-metacarpal level in an overnight broth culture of *Escherichia coli* K12 (mean CFU/ml=4.70x10<sup>8</sup>) for 5 seconds. The hands were then allowed to air dry for 3 minutes. Subsequently, the hands were sampled for pre-counts by massaging the fingertips in sterile Petri dishes containing 10ml tryptone soya broth (TSB) for 1 minute. The requisite volume of one of the three ABHR's was then added to the volunteers' hands with a calibrated pipette, and rubbed in using the standard hand rub procedure as described in EN1500 for 30 seconds. At the end of the rubbing procedure, the hands were sampled for post-counts by massaging the finger tips in sterile Petri dishes containing 10ml TSB for 1 minute. All samples were plated on to tryptone soya agar (TSA) with added deoxycholate and incubated at 37°C for 18 hours. Reduction factors were calculated by subtracting mean log<sub>10</sub> post-values from mean log<sub>10</sub> pre-values.

## RESULTS

•Figure 1 displays the spread of drying times per product, along with LOESS regression curves and 95% confidence intervals. The drying time for all three products increased as a function of volume. When calculated across all volumes, the mean drying time was 24.22 seconds for WHO1, 25.57 seconds for WHO2 and 28.32 seconds for 60% IPA. The only significant difference was between WHO1 and 60% IPA (p=0.030; Wilcoxon signed rank test).

•Figure 2 displays the user comments regarding drying time for the three products. The black dotted line represents the mean acceptable drying time, which was calculated across all three products as being equal to 25.33 seconds. There was a significant relationship between user acceptability and volume of application across all three products (p<0.001; Kruskal-Wallis rank sum test), with user acceptability being greatest around the 1.5ml and 2ml applications.

•Figure 3 shows the log<sub>10</sub> reduction factors produced by the different volumes of each product in the EN1500 -style test, along with line regression lines and 95% confidence intervals. More than 12 years' worth of EN1500 tests at HIRL have demonstrated that the reference product produces a mean log<sub>10</sub> RF of 5.16. This value is represented by the thick dotted line on Figure 3. The thin dotted line represents the agreed inferiority margin of 0.6 log<sub>10</sub> that is specified in EN1500. The log<sub>10</sub> RF's for all three products increased in a linear fashion as a function of volume. There was no significant difference between the mean log<sub>10</sub> RF's produced by each product, when calculated across all volumes (p=0.247; Friedman rank sum test).

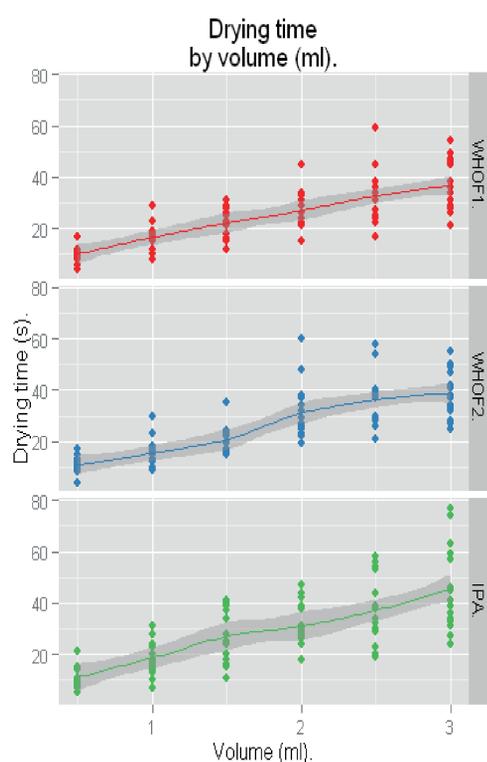


Figure 1

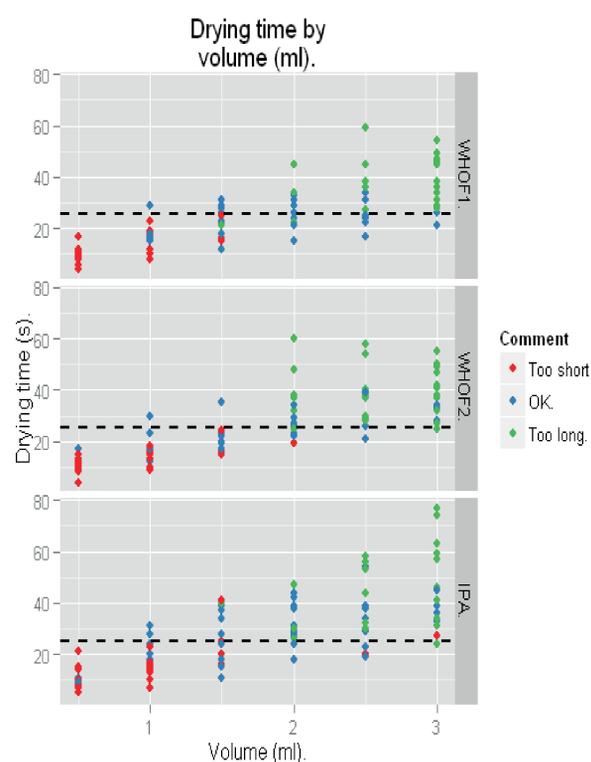


Figure 2

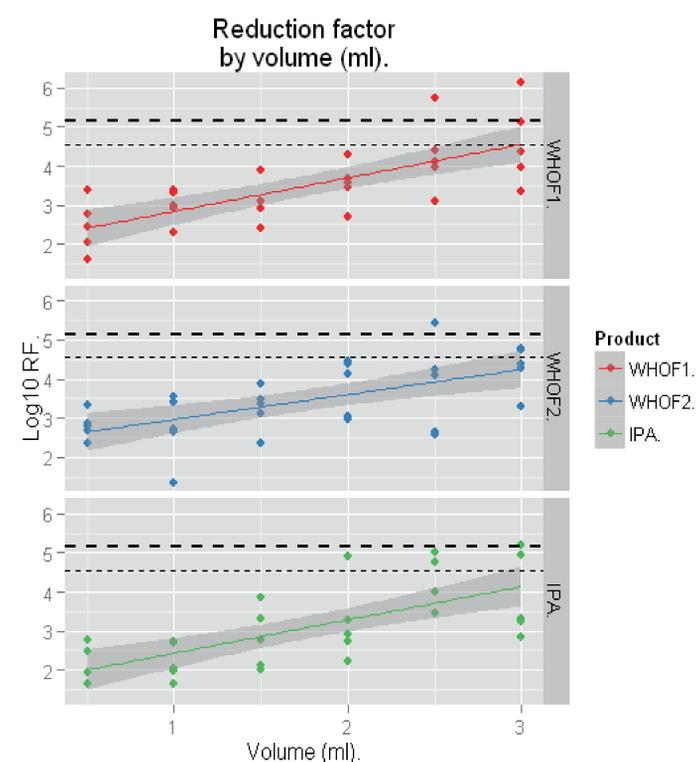


Figure 3

## CONCLUSION

EN1500 was not originally designed as a means to define product dosage; however this is increasingly becoming normal practice. The BPR requires manufacturers to support their label claims with data which is principally compliance with EN 1500. However, the data presented here reinforce the need for standards to reflect more accurately the volumes of hand rubs that are used in practice. The perception of the volunteers of an acceptable volume and drying time is in line with the WHO recommendations but would not comply with the requirements of EN 1500 even with the agreed inferiority margin of 0.6 log<sub>10</sub>. Similar results in relation to volume and drying time were recently published by Macinga et al<sup>3</sup>. Concerns have been expressed<sup>4</sup> that ABHRs applied as foams are unlikely to pass EN 1500, due to the low volumes often applied; the data presented here suggest that this is also true of liquid ABHRs when applied in realistic volumes.

One possible solution involves implementation of a phase 2 standard i.e. EN 1500 and a phase 3 test low volume/short drying times, thus allowing formulations to be tested against a reference product under both ideal and realistic conditions.

## REFERENCES

1. EN 1500:2013 Chemical disinfectants and antiseptics -Hygienic handrub-Test method and requirements (phase 2/step 2).
2. WHO Guidelines on Hand Hygiene in Health Care (2009). World Health Organization.
3. Macinga D, et al (2014) The relative influences of product volume, delivery format and alcohol concentration on dry-time and efficacy of alcohol-based hand rubs BMC Infectious Diseases 14: 511
4. Kampf G, Marschalls, Eggerstedt S, Ostermeyer C. (2010). Efficacy of ethanol-based hand foams using clinically relevant amounts: a cross-over controlled study among healthy volunteers. BMC Infectious Diseases. 10:78.

All materials for this study were funded by SC Johnson Professional. John Hines and Kevin Ormandy are employed by SC Johnson Professional. Research lead by Queen Elizabeth Hospital Birmingham. SC Johnson acquired Deb Group in 2015.